



## InterFlow™ Gas Blender

Specification sheet



Critical Care • Critical Care Equipment



## Application

Hospital use, continuous operation  
Suitable for adults, paediatrics and neonates

## Intended use

The InterFlow™ Gas Blender is intended to drive an air/oxygen blend at controlled flow and pressure to drive the required device for the chosen therapy. The InterFlow is intended for use with adult, paediatric and neonatal patients.

## Modes

**Adult CPAP:** Flow control mode intended to deliver CPAP therapy to adult patients via a Facemask.

**Adult Hood:** Flow control mode intended to deliver CPAP therapy to adult patients via a Hood.

**Adult HFOT:** Flow control mode intended to deliver HFOT (High Flow Oxygen Therapy) to adult patients via a High Flow nasal cannula.

Dimensions	
Size	H: 160 mm x W: 165 mm x D:110 mm
Weight	0.95 kg

Electrical rating	
Supply voltage	5V DC 500 mA
Supply frequency	50 – 60 Hz
Power rating	180-158 VA

Operating conditions	
Temperature	18°C to 26°C
Relative Humidity	10% to 80%
Atmospheric pressure	0 to 2,000m

Battery	
Type	Li-Ion
Operating time	0.5 hours
Capacity	3500 mAh, 12.6 Wh
Voltage	3.6V

Storage conditions	
Temperature	-18°C to 50°C
Relative Humidity	10% to 80%
Altitude	0 to 10,000m

Alarm volume	
High Priority	56 – 72 dB
Medium Priority	53 – 68 dB
Low Priority	54 – 69 dB

**Infant HFOT:** Flow control mode intended to deliver HFOT (High Flow Oxygen Therapy) to adult patients via a High Flow nasal cannula.

**Infant nCPAP – Flow:** Flow control mode intended to deliver nCPAP (nasal Continuous Positive Airway Pressure) to infant patients via an nCPAP generator.

**Infant nCPAP – Pressure:** Pressure control mode intended to deliver nCPAP (nasal Continuous Positive Airway Pressure) to infant patients via an nCPAP generator.

**Manual Flow:** Adjustable flow mode intended to allow the user maximum control of supplied flows.

Gas supply (STPD)	
O <sub>2</sub> supply	200 to 600 kPa; Medical oxygen
O <sub>2</sub> connection	NIST or DISS
Air supply	200 to 600 kPa; Medical air
Air connection	NIST or DISS

Performance (BTPS)	
O <sub>2</sub> %	21 – 100%
Flow	2 – 100 L/min
Pressure	0 – 210 cmH <sub>2</sub> O
Total System Response time	27 – 29s

Mechanical PRV	
Sustained pressure	< 330 cmH <sub>2</sub> O
Peak pressure	< 330 cmH <sub>2</sub> O

SD Card	
Type	Micro SD
Size	16GB
Read speed	>10MB/s
Class	4

System connections	
Gas outlet	22m/15F
Proximal pressure monitoring port	6% female luer

Noise emission	
Noise level	18°C toa <44 dB(A) 26°C




## Measurements

PI (perfusion index)**	
Range	0.02 - 20.0 %
Resolution	0.01 for < 10%; 0.1 for >= 10%
Accuracy	--
Flow (STPD)	
Range	0 - 100%
Resolution	0.1L/min
Accuracy	+- 10% cmH <sub>2</sub> O
Outlet Pressure	
Range	0 - 250 cmH <sub>2</sub> O
Resolution	0.1 cmH <sub>2</sub> O
Accuracy	+- 1 cmH <sub>2</sub> O
Patient Pressure	
Range	0 - 35 cmH <sub>2</sub> O
Resolution	0.1 cmH <sub>2</sub> O
Accuracy	± 0.3 cmH <sub>2</sub> O

O2*	
Range	0 - 100%
Resolution	0.1%
Accuracy	± 3 %
Data sample rate	5Hz
SpO2**	
Range	1 - 100%
Resolution	1%
Accuracy	± 3 digits (70 - 100%); unspecified (0 - 69%)
Data update period	1 s
Platform	Masimo®
Pulse**	
Range	25 - 240 b/min
Resolution	1 b/min
Accuracy	± 3%; ± 1b/min
Data update period	1 s

\* The oxygen sensor is filtered for accuracy with a response time of 3.2s. The maximum output response time from 21 – 90% oxygen is 90s.

\*\* Refer to IFU Section AA – 'Pulse Oximetry – Masimo SET®' for full details.

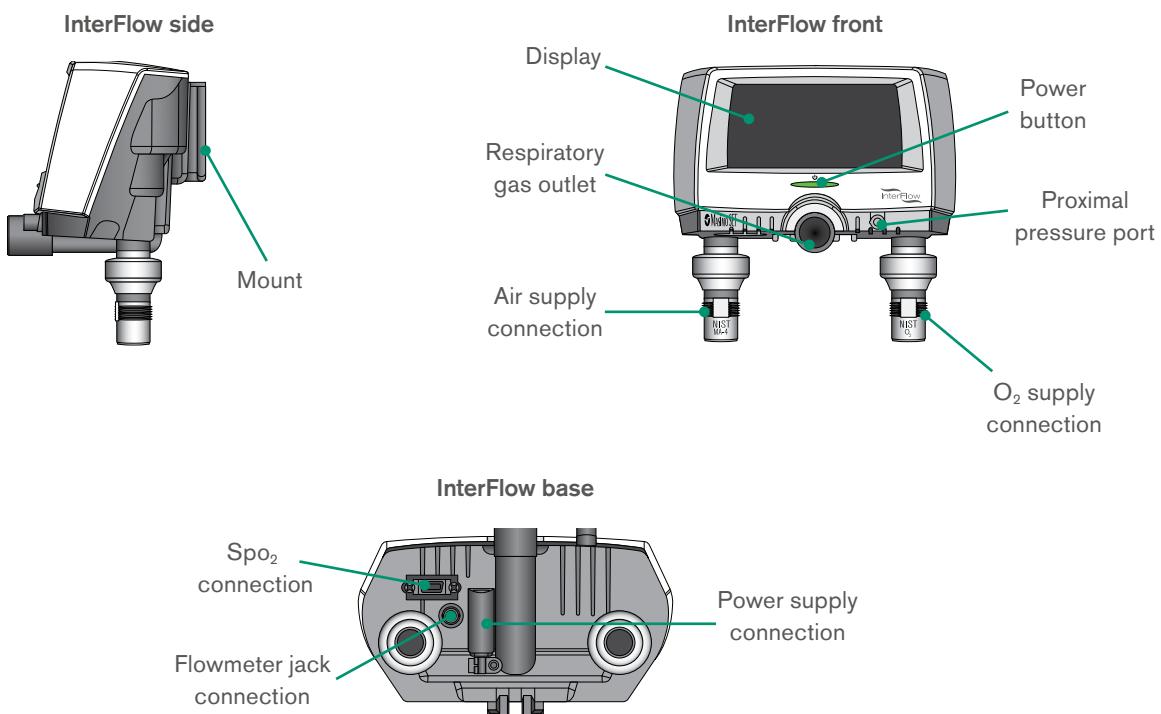



## Classifications

Protection class, electrical hazard	IEC 60601-1 Class II Medical Electrical Equipment.
Mode of operation	IP22 - Protected from touch by fingers and objects greater than 12 millimetres. Protected from water spray less than 15 degrees from vertical
Sterilisation	Do not sterilise
Applied Parts	This Device uses Type BF Applied Parts (Masimo SET® SpO2 sensors)

## Product standards

The InterFlow™ complies with the following relevant standards:

- ISO 60601-1
- ISO 80601-2-12
- IEC 60601-1-6
- ISO 80601-2-55
- IEC 60601-1-8
- ISO 80601-2-61
- IEC 60601-1-10
- ISO 11195

Masimo and Masimo SET are registered trademarks of Masimo Corporation.

## Mobile equipment stand



## Gas bottle kit



InterFlow spec sheet INT • Issue 2 09.25



Intersurgical Ltd, Crane House, Molly Millars Lane, Wokingham, Berkshire, RG41 2RZ, UK  
T: +44 (0)118 965 6300 info@intersurgical.com www.intersurgical.com



The manufacturer Intersurgical Ltd is certified to ISO 14001:2015, ISO 9001:2015, ISO 13485:2016 and MDSAP

### Please think before you print

Save energy and paper. If you must print this information sheet please print it double sided.